KEY
FLUID
ELEC. SIGNALS
ASA, INC. ITEMS

SAMPLE REQUIREMENTS:
(Without Filtering Accessories)

150 ppm TSS Maximum
60 NTU Maximum
5 Feet Max. Lift and 20 ft. run when using analyzer pump.

Filtering accessories available for sample points exceeding the above limits.

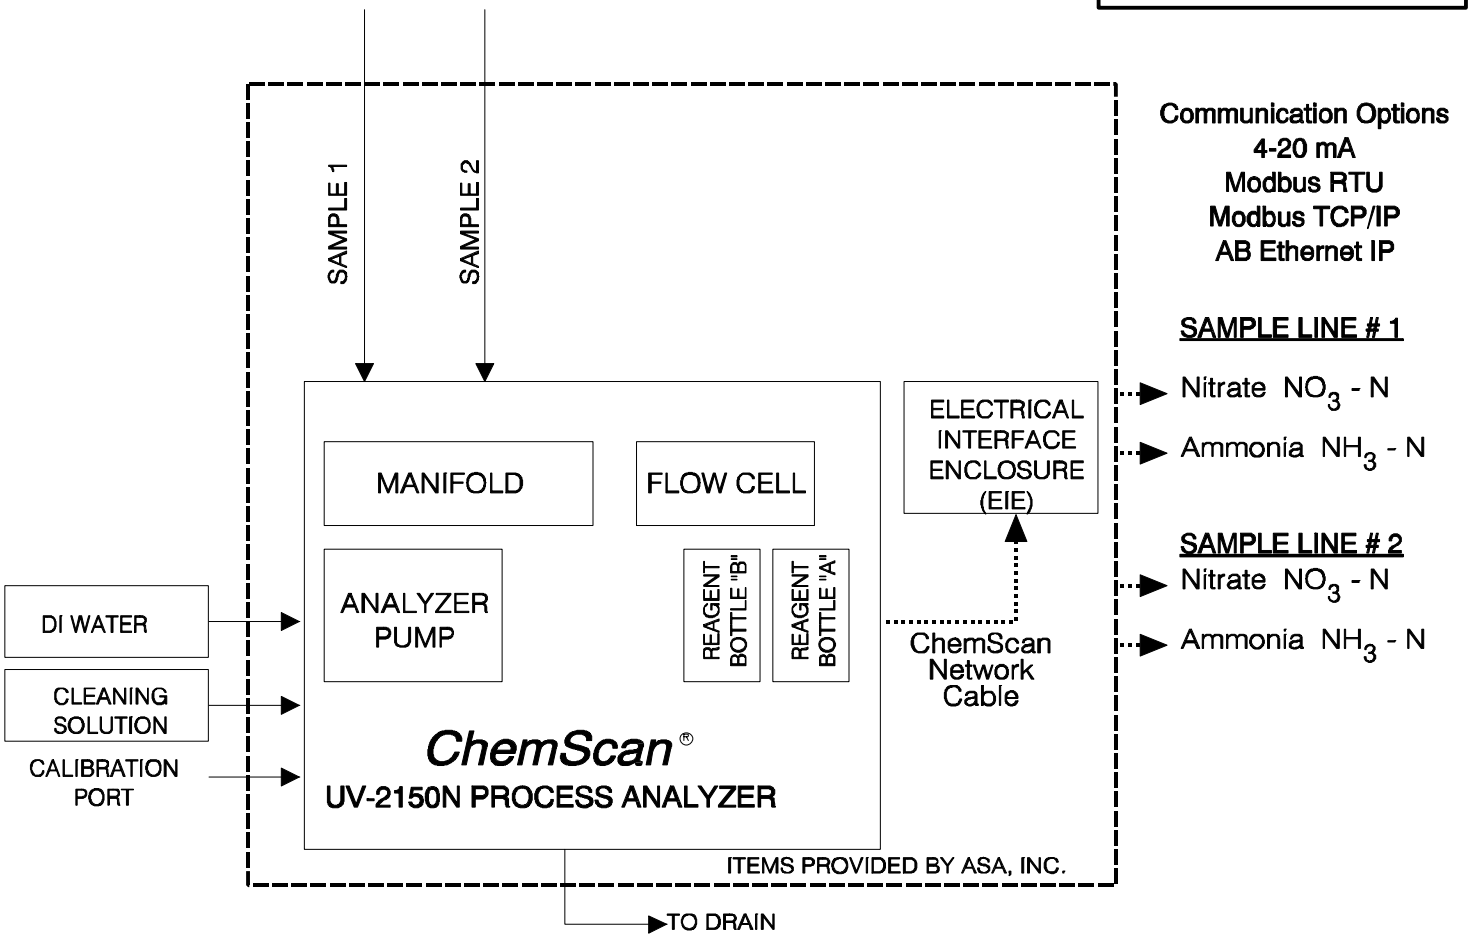

ChemScan®

Functional Block Diagram of Multi-Sample Line, Nitrate & Ammonia Monitoring System

ASA, Inc. PHONE: 262-717-9500 FAX: 262-717-9530

Applied Spectrometry Associates, Inc.©'09

DATE: 7/30/09 BY: LJB

Functional Block Diagram of Multi-parameter On-Line Monitoring System

FILE # 2N1SCBDA