


KEY	
—▶	FLUID
.....▶	ELEC. SIGNALS
- - - -	ASA, INC. ITEMS

**SAMPLE REQUIREMENTS:**  
 150 ppm TSS Maximum  
 60 NTU Maximum  
 5 Feet Max. Lift and 20 ft. run  
 when using analyzer pump

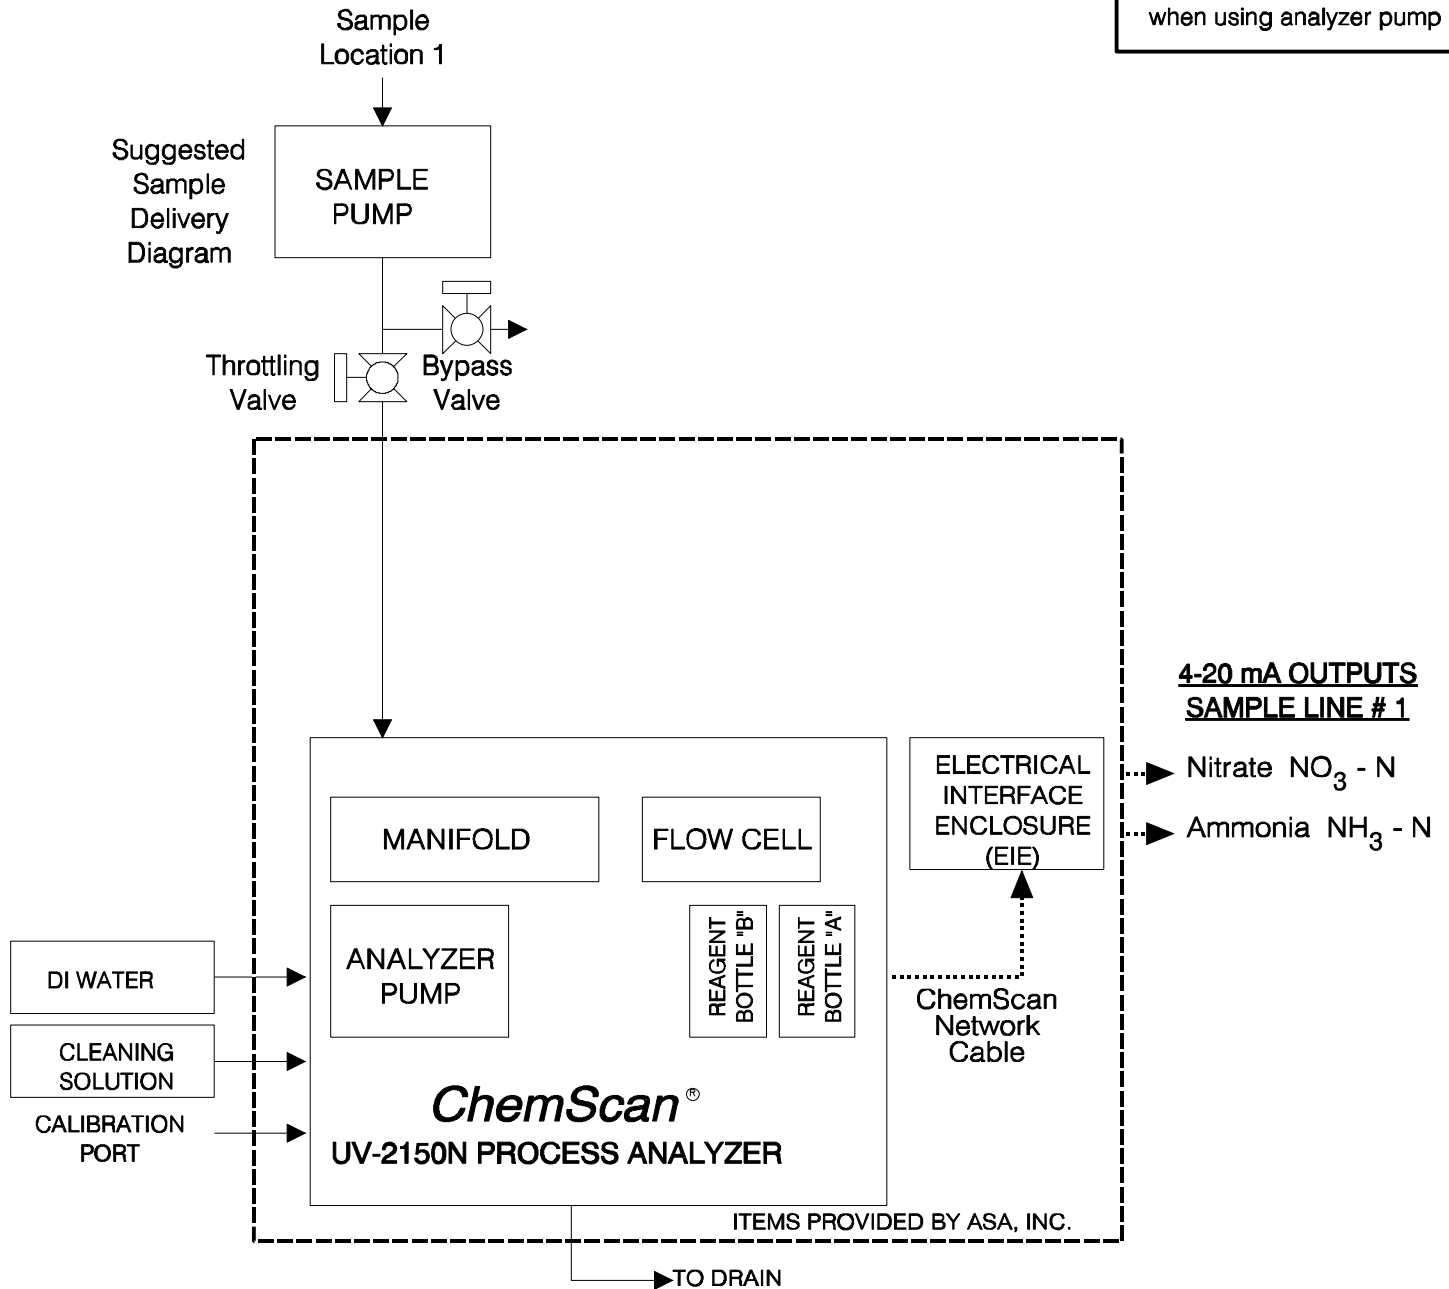

**ChemScan**<sup>®</sup>  
 Functional Block Diagram of  
 Monitoring System

<b>ASA, Inc.</b>	PHONE: 262-717-9500 FAX: 262-717-9530
Applied Spectrometry Associates, Inc. ©'09	
DATE: 7/30/09 BY: LJB	
Functional Block Diagram of Multi-parameter On-Line Monitoring System	
FILE # 2N1SCBDB	